

## Considering Thallium (TI)-201 SPECT MPI

Since 2009, there has been a global shortage of technetium (Tc)-99m, a widely used radiotracer for single-photon emission computed tomography (SPECT) myocardial perfusion imaging (MPI). This situation has led many nuclear labs to consider switching to thallium (TI)-201 protocols for SPECT MPI. Overall, TI-201 represents an acceptable alternative to Tc-99m, if labs make the necessary adjustments in terms of training, accreditation, equipment, and patient scheduling and care.

TI-201 is an analog of potassium with a physical half-life of 73 hours, high first-pass extraction, rapid clearance from the intravascular space, and redistribution that begins 10 to 15 minutes after injection.<sup>1</sup> These characteristics make TI-201 useful for assessing both myocardial blood flow and the viability of myocardial tissue; however, there are some disadvantages, such as somewhat poorer image quality and increased radiation burden.

### TI-201 PROTOCOLS

The most common TI-201 SPECT MPI protocol is stress/redistribution with optional reinjection.<sup>1</sup> TI-201 is injected just prior to peak exercise stress or at peak pharmacologic stress, and images are acquired 10 to 15 minutes later.<sup>1</sup> A redistribution (rest) study is then performed 2.5 to 4 hours later. If the images show a fixed defect, another redistribution study may be acquired at 18 to 24 hours to give a clearer determination of whether the defect is truly fixed or if the tissue is still viable.<sup>1</sup> It is particularly important to determine the viability of a fixed defect if the patient has had a previous myocardial infarction (MI).<sup>2</sup> Another option to assess viability is to reinject with 1-2 mCi TI-201 immediately after the first redistribution study, and then acquire another image.<sup>1</sup> This allows the protocol to be completed in 1 day, but exposes the patient to a higher radiation dosage.

The dual-isotope protocol uses a small quantity of Tc-99m for the stress image and TI-201 for the rest image.<sup>1</sup> This protocol may help conserve existing supplies of Tc-99m, and it takes advantage of the favorable properties of each tracer—blood flow assessment with Tc-99m and viability assessment with TI-201.<sup>3</sup> Imaging in this manner provides valuable information on viability, particularly for patients with previous MI or heart failure.<sup>1</sup> Again, however, the radiation burden to the patient is substantially higher with dual isotope than with Tc-99m protocols.

### CAMERA PARAMETERS

Labs that usually use Tc-99m will need to make some adjustments to their camera parameters in order to perform TI-201 SPECT MPI. The best TI-201 images are usually achieved using a low-energy all-purpose (LEAP) SPECT collimator, as opposed to the low-energy high-resolution (LEHR) collimator used with Tc-99m.<sup>4</sup> Some older labs may have both collimators on hand, in which case they can simply be switched out for TI-201 studies. LEHR collimators can still be used, but time per projection must be increased.<sup>5</sup> In addition, TI-201 images require more filtering. Scanner configuration, reconstruction algorithms, radionuclide doses, and patient populations vary between

laboratories,<sup>4</sup> so each lab should select camera parameters in consultation with the interpreting physician. Table 1 lists the optimum camera parameters for the TI-201 stress/redistribution protocol.<sup>4</sup> TI-201 produces lower counts and has a higher incidence of tissue attenuation, and thus more scatter radiation.<sup>4</sup> For these reasons, images generally will not be as clear as those of Tc-99m, and may require readjustment by the reading physician.

**Table 1. Camera parameters for stress/redistribution TI-201 acquisition.**

Parameter	Stress study	Redistribution (rest) study	Guideline
Dose	2.5-3.5 mCi TI-201	Not applicable	Standard
Position	Supine	Same	Standard
	Prone	Same	Optional
	Upright/Semiupright	Same	Optional
Delay time (Injection→imaging)	10-15 minutes <sup>a</sup>	Not applicable	Standard
Delay time (Stress→rest)	Not applicable	3-4 hours	Standard
Energy windows	30% symmetric, 70 keV 20% symmetric, 167 keV	Same	Standard
Collimator	LEAP	Same	Preferred
Orbit	180° (45° RAO to 45° LPO)	Same	Preferred
Orbit type	Circular	Same	Standard
	Noncircular	Same	Standard
Pixel size	6.4 ± 0.4 mm	Same	Standard
Acquisition type	Step and shoot	Same	Standard
	Continuous	Same	Optional
Number of projections	32-64	Same	Standard
Matrix	64 x 64	Same	Standard
Time/projection	40 s (32 fr), 25 s (64 fr)	Same	Standard


RAO=right anterior oblique; LPO=left posterior oblique

<sup>a</sup> An anterior planar image may be acquired during this interval to evaluate TI-201 lung uptake.

## LOGISTICS AND SCHEDULING

Switching to TI-201 will also require changes to scheduling and office logistics. Because TI-201 images must be acquired 10 to 15 minutes after injection,<sup>1</sup> patients will need to be injected in close proximity to the scanner. A delay of at least 10 minutes is required to avoid upward-creep artifacts, which can lead to false-positive findings.<sup>5</sup> Scheduling will need to account for the fact that there is no “lag time” between injection and imaging, as there is with Tc-99m. In addition, the redistribution study is performed 2.5 to 4 hours later, and there may be a reinjection image performed that day, or another redistribution image performed the following day.

**Figure 1. Patient radiation exposure from various MPI protocols.**

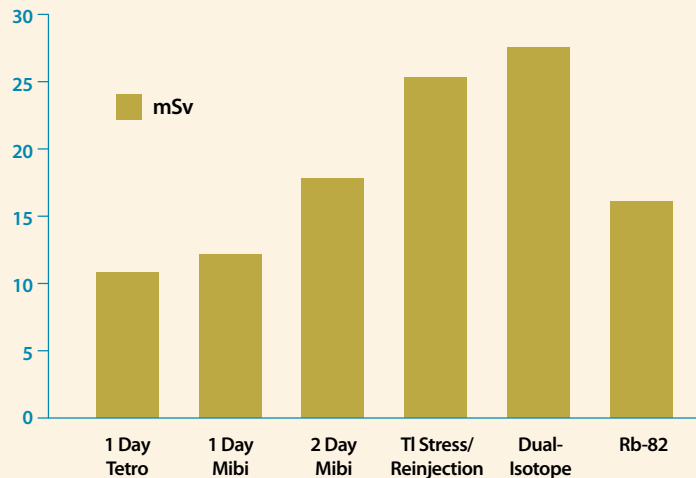

Adapted from Thompson R, et al. *J Nucl Cardiol.* 2006;13:19-23.

## RADIATION EXPOSURE

As mentioned earlier, the major drawback to TI-201 SPECT MPI is the increased radiation burden. The dual-isotope protocol gives an approximate patient radiation dosage of 27.3 mSv, the highest among common cardiovascular radionuclide imaging studies.<sup>6</sup> The TI-201 stress/redistribution/reinjection protocol is almost as high, at 25.1 mSv.<sup>6</sup> In comparison, the 3 most common Tc-99m protocols have dosages of 10.6 mSv, 12 mSv, and 17.5 mSv (see Figure 1).<sup>6</sup>

## TRAINING AND ACCREDITATION

To perform TI-201 SPECT protocols, a nuclear lab's US Nuclear Regulatory Commission (NRC) or Agreement State license must include the TI-201 radiotracer, or be a broad scope license.<sup>7</sup> Otherwise, the license will need to be amended.<sup>8</sup> In addition, the American College of Radiology (ACR) accreditation requires that each SPECT scanner be accredited for each isotope to be used on that scanner.<sup>9</sup>

If a lab is currently accredited with the Intersocietal Commission for the Accreditation of Nuclear Laboratories (ICANL) and has the proper license, switching to TI-201 protocols should have very little effect on lab accreditation. Although most US nuclear labs stopped using TI-201 after Tc-99m-labeled sestamibi was approved by the Food and Drug Administration in 1991,<sup>10</sup> nuclear cardiologists, nurses, and technologists should have had some general background training

Visit [pharmstresstech.com](http://pharmstresstech.com) for interactive *Tech Tips* modules that include additional data and a question and answer section that may be useful educational tools.

based on appropriate reading and review of case files, in the absence of hands-on experience with TI-201 SPECT MPI.<sup>11</sup> To ensure that a lab is accredited by ICANL to perform TI-201 imaging, the Medical Director is required to create a written protocol detailing how the lab will image with TI-201 prior to performing the first study.<sup>12</sup> The protocol should be in compliance with guidelines published by professional societies. Labs are not required to submit that protocol to the ICANL—they are only required to have it available.<sup>13</sup>

## ISSUES RELATED TO LONGER HALF-LIFE

Due to its longer half-life, it will take longer for stored TI-201 to decay to background levels than Tc-99m. Labs should check with their NRC or Agreement State regulations regarding the disposal of nuclear waste in their jurisdiction. In addition, TI-201 may remain detectable in the body for up to 30 days postinjection, so patients who will be traveling after receiving TI-201 SPECT MPI may need a note from the lab explaining their unusually high radiation levels.<sup>14</sup>

## CONCLUSIONS

In the wake of the global Tc-99m shortage, many nuclear labs are considering the use of TI-201 for SPECT MPI. TI-201 protocols provide valuable data on myocardial blood flow and viability, though with higher radiation dosage and somewhat lower-quality images. Camera parameters, logistics, and scheduling in the nuclear lab will likely need to change to accommodate TI-201. As long as the proper license is held, maintaining ICANL accreditation with TI-201 should not be difficult. TI-201 protocols are an acceptable alternative to Tc-99m.

**For more information on TI-201, visit the following Web sites:**

**ASNC** – TI-201 Protocols, Guidelines, and Standards  
[http://www.asnc.org/section\\_73.cfm](http://www.asnc.org/section_73.cfm)

**ASNC** – Resources and Educational Programs  
[http://www.asnc.org/content\\_550.cfm](http://www.asnc.org/content_550.cfm)

**NRC** – Licensing  
<http://www.nrc.gov/materials/medical.html>

**References:** 1. Henzlova MJ, Cerqueira MD, Mahmarian JJ, Yao S-S. Stress protocols and tracers. *J Nucl Med Cardiol.* 2006;13:e80-e90. 2. Van Eck-Smit B, Van Der Wall E, Siebelink H-MJ, Baur L, Zwinderman A, Pauwels E. Head-to-head comparison of 201Tl rest-redistribution scintigraphy and stress-immediate reinjection scintigraphy in the detection of myocardial viability. *Nucl Med Commun.* 1996;17:216-224. 3. Dilsizian V. SPECT and PET Imaging: Tracers and Techniques. In: Dilsizian V, Narula J, eds. *Atlas of Nuclear Cardiology.* 2nd ed. Philadelphia, PA: Current Medicine LLC; 2006:43. 4. Holly T, Abbott B, Al-Mallah M, et al. ASNC imaging guidelines for nuclear cardiology procedures: Single-photon emission computed tomography [published online June 15, 2010]. *J Nucl Cardiol.* <http://asnc.org/imageuploads/ImagingGuidelineSPECTJune2010.pdf>. Accessed August 4, 2010. 5. Pagnanelli RA, Basso DA. Myocardial Perfusion Imaging with 201Tl. *J Nucl Med Technol.* 2010;38:1-3. 6. Thompson R, et al. Issues regarding radiation dosage of cardiac nuclear and radiography procedures. *J Nucl Cardiol.* 2006;13:19-23. 7. Nuclear Regulatory Commission. NRC Regulations, Title 10, Code of Federal Regulations, Part 33. *Fed Regist.* <http://www.nrc.gov/reading-rm/doc-collections/cfr/part033/>. Updated June 23, 2010. Accessed August 4, 2010. 8. Nuclear Regulatory Commission. NRC Regulations, Title 10, Code of Federal Regulations, Part 35. *Fed Regist.* <http://www.nrc.gov/reading-rm/doc-collections/cfr/part035/>. Updated June 23, 2010. Accessed August 4, 2010. 9. ACR Nuclear Medicine/PET Accreditation Program Requirements. American College of Radiology Web site. [http://acr.org/accreditation/nuclear/nuc\\_med\\_reqs.aspx](http://acr.org/accreditation/nuclear/nuc_med_reqs.aspx). Accessed September 22, 2010. 10. Strauss HW, Bailey D. Resurrection of Thallium-201 for Myocardial Perfusion Imaging. *JACC Cardiovasc Imaging.* 2009;2:283-285. 11. Cerqueira M, Berman D, Di Carli M, Schelbert H, Wackers F, Williams K. ACCF COCATS 3 training statement: Task Force 5: Training in nuclear cardiology. *JACC.* 2008;51:368-374. 12. The Complete 2010 ICANL Standards for Nuclear Cardiology, Nuclear Medicine and PET Accreditation. ICANL Web site. [http://www.icanl.org/icanl/standards/2010\\_ICANL\\_Standards.pdf](http://www.icanl.org/icanl/standards/2010_ICANL_Standards.pdf). Accessed August 4, 2010. 13. Intersocietal Commission for the Accreditation of Nuclear Medicine Laboratories. Emerging technologies. ICANL Web site. <http://icanl.org/icanl/community/qaspp.htm>. Accessed August 4, 2010. 14. Nuclear Medicine Patients: No-Alarm Holiday Travel Tips [press release]. SNM Web site. <http://interactive.snm.org/index.cfm?PageID=5660>. Published November 9, 2006. Accessed September 22, 2010.

Provided as an educational service by **Astellas Pharma US, Inc.**

COMMITTED TO CARDIOLOGY™